






# Pile Dynamics, Inc.

## Transducer C070

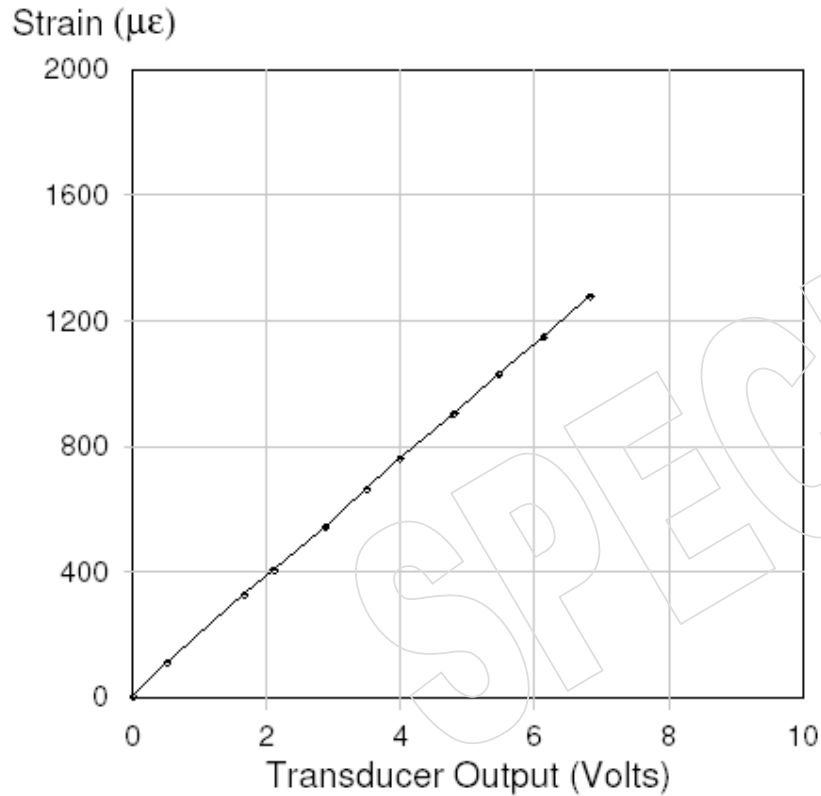

PDA Cal Factor (5.0 V) 93.0 $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
111	0.51
327	1.65
406	2.10
542	2.87
665	3.49
760	3.99
904	4.80
1029	5.46
1147	6.12
1277	6.82

Shunt (60.4 K $\Omega$ ) 2.5 V  
 General Factor 323.0 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by: \_\_\_\_\_  
 Calibrated on: 12-Mar-2009